



## ISTITUTO NAZIONALE DI RICERCA METROLOGICA Repository Istituzionale

1337 EURAMET.EM.M.S2

SUPPLEMENTARY COMPARISON OF NATIONAL STANDARD FACILITIES IN THE FIELD OF

This is the author's submitted version of the contribution published as:

*Original*

1337 EURAMET.EM.M.S2

SUPPLEMENTARY COMPARISON OF NATIONAL STANDARD FACILITIES IN THE FIELD OF MEASURING THE POLARIZATION AND SPECIFIC TOTAL POWER LOSS IN SOFT MAGNETIC MATERIALS

FINAL REPORT / Albrecht, M.; Kupec, M. A. Malygin. J.; Ulvr, M.; Appino, C.; Hall, M.; Turner, S.. - In: METROLOGIA. - ISSN 0026-1394. - Technical Supplement:01006(2018), pp. 1-17.

*Availability:*

This version is available at: 11696/60003.5 since: 2021-02-06T17:49:37Z

*Publisher:*

BIPM

*Published*

DOI:

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

(Article begins on next page)



SUPPLEMENTARY COMPARISON OF NATIONAL STANDARD FACILITIES IN THE FIELD  
OF MEASURING THE POLARIZATION AND SPECIFIC TOTAL POWER LOSS IN SOFT  
MAGNETIC MATERIALS

REPORT A

**Pilot laboratories:**

AG 2.51 “Magnetic measurements”  
Physikalisch-Technische Bundesanstalt  
Bundesallee 100  
38116 Braunschweig  
Germany  
Contact Person:  
Martin Albrecht  
Tel.: +49 531 592 2250, FAX +49 592 2205  
E-mail: martin.albrecht@ptb.de

Laboratory of metrology of magnetic and acoustic quantity (261)  
“Urals Scientific Research Institute of Metrology”  
(FGUP “UNIIM”) Russia, Yekaterinburg  
620000 Russia Yekaterinburg  
Krasnoarmeyskaya Str, 4  
Contact person:  
Malygin Michael Aleksandrovich  
Tel/Fax (343) 355-38-92  
E-mail: maligin@uniim.ru

## Introduction

At a meeting at the PTB in Braunschweig on the 5th and 6th of March 2014 between the representatives of UNIIM (Russia), **PTB** (Germany), CMI (Czech Republic), NPL (United Kingdom) the decision was made to carry out a supplementary comparison for the measurement of specific total power loss in soft magnetic materials. The measurements were done in compliance to IEC 60404 part 2 on a defined set of magnetic materials supplied by UNIIM and NPL. An additional participant is INRIM (Italy).

Two work items have been defined:

- First: the results of the measurements shall demonstrate the degree of equivalence between the laboratories.
- Second: the capability of the test equipment shall be compared.

### CMC classification numbers:

12.3.1 Specific total power loss: Epstein, ring and single sheet sample

## 1. Participants

Table 1 – The list of participants of comparisons

№	Country	Address	Organization	Participant Name	Contact Information
1	Russia	620000, Russia, Yekaterinburg, Krasnoarmeyskaya Str, 4	UNIIM	Malygin Michael Aleksandrovich	E-mail: maligin@uniim.ru Tel/Fax: +7 343 355-38-92
2	Germany	Bundesallee 100 38116 Braunschweig Germany	PTB	Martin Albrecht	E-mail: martin.albrecht@ptb.de
3	Czech Republic	Czech Republic, V Botanice 4, Praha 5 15072	CMI	Josef Kupec Michal Ulvr	E-mail: jkupec@cmi.cz
4	Italy	Strada delle Cacce 10135 Torino ITALY	INRIM	Carlo Appino	E-mail: c.appino@inrim.it Tel: +390113919841 Fax: +390113919834
5	United Kingdom	Hampton Road, Teddington, Middlesex, TW11 0LW.	NPL	Michael Hall Steven Turner	E-mail: steven.turner@npl.co.uk

## **2. Organization of the comparisons**

### **2.1 Organization of the comparisons**

The Comparison is carried out by a circulation scheme. Standard samples were produced by UNIIM (Russia) by May 2014 and measured with  $\mu\mu\mu$  198-2011. After initial measurements at UNIIM one set of each sample and the single NPL ring core were sent to: 1. PTB, 2. CMI, 3. INRIM, 4. NPL, and after this returned to UNIIM for final measurements to establish the stability (except NPL ring core). After measurements the data were sent to UNIIM for evaluation of the comparison results.

### **2.2 The transfer standard**

Four samples were used for comparisons:

2 Epstein samples (UNIIM);

1 ring sample for comparison (UNIIM); and

1 ring sample for the comparison of the electrical measurements (NPL).

For the transfer standards provided by UNIIM three sets of each sample were prepared. Two sets stay at UNIIM and one set is distributed around the participants for the measurements of the comparison. Two sets are kept in reserve in case of damage to samples being circulated.

The transfer standards are samples of grain oriented and non-oriented electrical steel:

- one sample (No 1) of non-oriented steel in the form of strips with the dimensions (30 $\mu$ 280) mm for Epstein frame measurements with a weight of approximately 0.5 kg and thickness of approximately 0.35 mm. The quantity of the strips in the sample must be a multiple of 4;
- one sample (No 2) of grain oriented steel in the form of strips with the dimensions (30 $\mu$ 280) mm for Epstein frame measurements with a weight of approximately 0.5 kg, and thickness of approximately 0.23 mm. The quantity of the strips in the sample must be a multiple of 4;
- one ring sample made by a method of stamping of rings from grain oriented steel with the primary and secondary winding placed on the core and fixed firmly in position.
- one ring sample made of non-oriented steel with known characteristic supplied by NPL.

Samples are packed in wooden boxes for their safety during transportation.

## **3. Description of the method of measurement**

During the comparisons measurements are carried out using the measurement standards of National Metrological Institutes (NMI).

### **3.1 Epstein samples**

#### **3.1.1 Preparation of the transfer samples for measurements**

The sample in the form of strips with sizes 30x280 mm should be loaded into the Epstein frame in accordance with figure 1. On each strip an index showing the position within the pack and an arrow specifying position of the strip in the solenoids of the Epstein frame. The strips 1.1 and 3.1 are placed in solenoids 1 and 3 of the Epstein frame first. The solenoids 1 and 3 of the Epstein frame are parallel. The strips 2.1 and 4.1 are placed in the solenoids 2 and 4 of the Epstein frame. This sequence is repeated until all strips are loaded into the frame.

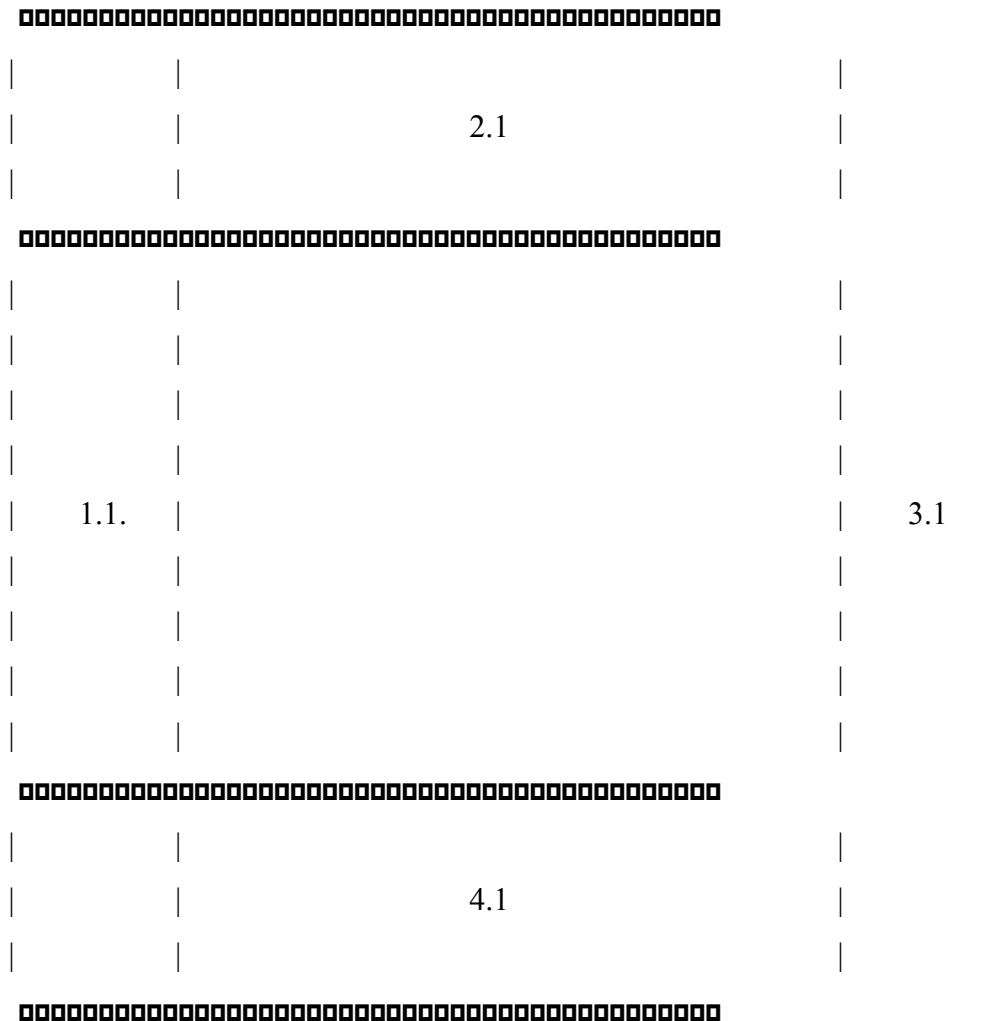


Figure 1 – Method of loading strips in the Epstein frame.

When loading the non-oriented steel, strips cut with the rolling direction should be loaded into two parallel solenoids with the strips cut against the rolling direction loaded into the other two solenoids.

The sample is demagnetized by a variable magnetic field with a frequency of 50 Hz and with decreasing amplitude starting from a peak polarization larger than that used for measurements to a value as close as possible to zero. This should be not less than 1.8 T for an grain-oriented steel and not

less than 1.6 T for an non-oriented steel. The time taken for the demagnetization should be not less than 40 s.

This demagnetization should be performed before each series of measurements.

### 3.1.2 Measurements of the Epstein samples

Each participant performs the following measurements using their standard equipment and measurement procedure:

The specific total loss and specific apparent power are measured stepwise from the lowest to the highest peak polarization value given below. At these values of peak magnetic polarization the values of the peak magnetic field strength are measured simultaneously (preferably).

Parameters for Epstein sample No 1 (non-oriented):

Frequency 50 Hz, 60 Hz

Magnetizing curve  $J_{\max} = F(H_{\max})$

$H_{\max} = 100, 200, 500, 1000, 2500, \text{ A/m.}$

Specific loss  $P = F(J_{\max})$

at  $J_{\max} = 1.0; 1.1; 1.3; 1.5; 1.6 \text{ T.}$

Parameters for Epstein sample No 2 (grain oriented):

Frequency 50 Hz, 60 Hz

Magnetizing curve  $J_{\max} = F(H_{\max})$

at  $H_{\max} = 30, 100, 500, 1000, 1500 \text{ A/m.}$

Specific loss  $P = F(J_{\max})$

at  $J_{\max} = 1.0; 1.3; 1.5; 1.7; 1.8 \text{ T.}$

## 3.2 Ring samples

### 3.2.1 Preparation of the ring samples

The sample is connected to the measurement setup used for this comparison. The sample is demagnetized by a variable magnetic field with frequency 50 Hz and with decreasing amplitude starting from a peak polarization larger than that used for measurements to a value as close as possible to zero. This should be not less than 1.8 T for grain-oriented steel and not less than 1.6 T for non-oriented steel. The time taken for the demagnetization should be not less than 40 s.

This demagnetization should be performed before each series of measurements.

### 3.2.2 Measurements of the ring samples

On the ring samples the specific total power loss and specific apparent power are measured stepwise from the lowest to the highest value given below. At the same values of the peak total

magnetic flux density,  $B$ , the values of the peak magnetic field strength are measured simultaneously (preferably).

Parameter sets for the measurements on the grain oriented ring:

1. Frequency 50 Hz, 60 Hz  
Magnetizing curve  $J_{\max} = F(H_{\max})$   
at  $H_{\max} = 30, 100, 500, 1000, 1500$  A/m.  
Specific loss  $P = F(J_{\max})$   
at  $J_{\max} = 1.0; 1.3; 1.5; 1.7; 1.8$  T
2. Frequency 400 Hz,  
Magnetizing curve  $J_{\max} = F(H_{\max})$   
at  $H_{\max} = 30, 100, 500, 1000, 1300$  A/m.  
Specific loss  $P = F(J_{\max})$   
at  $J_{\max} = 1.0; 1.3; 1.5; (1.6; 1.7)$  T
3. Frequency 1000 Hz if possible,  
Magnetizing curve  $J_{\max} = F(H_{\max})$   
at  $H_{\max} = 30, 100, 300, 500$  A/m.  
Specific loss  $P = F(J_{\max})$   
at  $J_{\max} = 0.5; 0.7; 1.0$  T

Parameters for the NPL ring core manufactured from non-oriented Transil grade steel:

Frequency 50 Hz, 60 Hz  
Magnetizing curve  $J_{\max} = F(H_{\max})$   
 $H_{\max} = 100, 200, 500, 1000$  A/m.  
Specific loss  $P = F(J_{\max})$   
at  $J_{\max} = 1.0; 1.1, 1.3; 1.5; 1.6$  T.

#### **4. The results of comparisons**

##### **4.1 The results of measurements and a standard uncertainty of measurement results (%) of the sample from non-oriented electrical steel $\square 1$ with the following characteristics:**

total weight – 0.5480 kg  
effective mass – 0.4599 kg  
sample length – 0.280 m  
cross sectional area –  $6.396 \cdot 10^{-5}$  m<sup>2</sup>  
density – 7650 kg/m<sup>3</sup>

with Epstein tester are shown in Table 1.

**4.2 The results of measurements and a standard uncertainty of measurement results (%) of the sample from grain-oriented magnetic steel  $\alpha 2$  with the following characteristics:**

total weight – 0.5082 kg

effective mass – 0.4265 kg

sample length – 0.280 m

cross sectional area –  $5.931 \cdot 10^{-5} \text{ m}^2$

density –  $7650 \text{ kg/m}^3$

with Epstein tester are shown in Table 2.

**4.3 The results of measurements and a standard uncertainty of measurement results (%) of the ring sample from grain-oriented magnetic steel  $\alpha 18$  with the following characteristics:**

total weight – 0.2393 kg

length of magnetic path – 0.18064 m

cross sectional area –  $1.732 \cdot 10^{-4} \text{ m}^2$

density –  $7650 \text{ kg/m}^3$

are shown in Table 3.

**4.4 The results of measurements and a standard uncertainty of measurement results (%) of the ring sample from non-oriented magnetic steel T1002 with the following characteristics:**

total weight – 0.5075 kg

length of magnetic path – 0.44061 m

cross sectional area –  $1.503 \cdot 10^{-4} \text{ m}^2$

density –  $7650 \text{ kg/m}^3$

are shown in Table 4

**5 Processing of results**

Processing of measurement results obtained from the comparisons carried out with the use of the Guidelines for data evaluation of COOMET supplementary comparisons (COOMET R/GM/19:2008) and the Guidelines for data evaluation of COOMET key comparisons (COOMET R/GM/14:2006).



In processing the experimental data following characteristics were calculated:

- supplementary comparisons reference value  $X_{ref}$  by the formula:

$$X_{ref} = \frac{\sum_{i=1}^N \frac{X_i}{u^2(X_i)}}{\sum_{i=1}^N \frac{1}{u^2(X_i)}}, \quad (1)$$

where  $X_i$  – results of the supplementary comparisons of the  $i$ -th participant of the comparisons;

$u(X_i)$  – declared standard uncertainty of the  $i$ -th participant of the comparisons, %;

$N$  – the number of the participants of comparisons;

- standard uncertainty of the reference value of the supplementary comparisons  $u(X_{ref})$ , % by the formula:

$$u(X_{ref}) = \sqrt{\frac{1}{\sum_{i=1}^N \frac{1}{u^2(X_i)}}} \quad (2)$$

- degree of equivalence of the  $i$ -th participant of the comparisons by the formulas 3, 4 and 5:

$$d_i = X_i - X_{ref} \quad (3)$$

$$u^2(d_i) = u^2(X_i) + u^2(X_{ref}) \quad (4)$$

$$E_n = \frac{|d_i|}{2 u(d_i)}, \quad (5)$$

where  $d_i$  – degree of equivalence;

$u(d_i)$  – standard uncertainty of the degree of equivalence.

The declared uncertainties are judged as confirmed if equation  $E_{Hi} < 2$  is satisfied, that is a confirmation of the relevant rows from CMC.

The results of calculations by the formulas 1 and 2 are shown in Tables 2-5.

The results of calculations by the formulas 3-5 are shown in Tables 6-9.

## 6 Evaluation of the comparisons results

After the evaluation of the data in agreement with the rules of EURAMET the agreement of the comparison seems to be good. The data of NMIs participating in the comparisons can be judged as concerted that is an objective confirmation of the declared uncertainties.

There is one exception for all participants for the measurement on a grain-oriented ring sample at high frequencies. The results show clearly that the measurement equipment used for this kind of samples is not suited to get consistent results. Thus, there is further work necessary to get equipment suited for higher frequencies. Until this is done, the uncertainties of all participants for these values have to be increased significantly!

Table 2. The results of measurements and a standard uncertainty of measurement results of the sample □ 1

Parameter	CMI, Czech Republic		PTB, Germany		INRIM, Italy		NPL, United Kingdom		UNIIM, Russia		$\bar{X}_{ref}$	$u^2(\bar{X}_{ref})$	$u_{\bar{X}_{ref}}$
	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$			
P <sub>1,0/50</sub> (W/kg)			0,9481	0,2	0,959	0,53	0,942	0,325	0,9479	0,52	0,9476	0,0240	0,1548
P <sub>1,1/50</sub> (W/kg)	1,1206	0,5	1,1306	0,203	1,141	0,58	1,126	0,325	1,1336	0,6	1,1305	0,0180	0,1343
P <sub>1,3/50</sub> (W/kg)			1,6116	0,243	1,621	0,62	1,607	0,325	1,6098	0,42	1,6108	0,0288	0,1698
P <sub>1,5/50</sub> (W/kg)			2,3036	0,243	2,3	0,82	2,288	0,375	2,2998	0,36	2,2992	0,0301	0,1734
P <sub>1,0/60</sub> (W/kg)			1,1969	0,2	1,213	0,48	1,189	0,325	1,193	0,5	1,1964	0,0234	0,1528
P <sub>1,1/60</sub> (W/kg)	1,3993	0,5	1,4272	0,203	1,44	0,55	1,422	0,325	1,4254	0,5	1,4269	0,0244	0,1561
P <sub>1,3/60</sub> (W/kg)	1,9864	0,5	2,0319	0,241	2,05	0,58	2,026	0,325	2,0295	0,36	2,0313	0,0268	0,1636
P <sub>1,5/60</sub> (W/kg)	2,87	0,5	2,9043	0,238	2,917	0,82	2,886	0,375	2,9025	0,38	2,9006	0,0301	0,1736
100/50 (T)	-		0,9943	0,141	0,988	0,29	1,001	0,26	1,0006	0,6	0,9948	0,0125	0,1120
200/50 (T)	-		1,2352	0,121	1,232	0,29	1,237	0,225	1,2355	0,46	1,2352	0,0096	0,0977
500/50 (T)	1,3667	0,5	1,3719	0,117	1,3696	0,27	1,373	0,225	1,3713	0,38	1,3718	0,0077	0,0879
1000/50 (T)	1,435	0,5	1,4395	0,118	1,4369	0,26	1,44	0,225	1,4395	0,32	1,4393	0,0076	0,0870
2500/50 (T)	1,5327	0,5	1,5352	0,117	1,5353	0,26	1,537	0,225	1,5359	0,3	1,5356	0,0074	0,0862
100/60 (T)	-		0,9934	0,142	0,9831	0,29	0,999	0,26	1,0006	0,6	0,9932	0,0126	0,1125
200/60 (T)	-		1,236	0,12	1,2286	0,29	1,237	0,225	1,2355	0,46	1,2353	0,0095	0,0972
500/60 (T)	1,3683	0,5	1,373	0,116	1,3708	0,27	1,373	0,225	1,3713	0,38	1,3726	0,0077	0,0875
1000/60 (T)	1,4378	0,5	1,4407	0,116	1,4381	0,26	1,441	0,225	1,4395	0,32	1,4403	0,0074	0,0862
2500/60 (T)	1,5351	0,5	1,5366	0,117	1,5364	0,26	1,536	0,225	1,5359	0,3	1,5364	0,0074	0,0862

Table 3. The results of measurements and a standard uncertainty of measurement results of the sample □ 2

Parameter	CMI, Czech Republic		PTB, Germany		INRIM, Italy		NPL, United Kingdom		UNIIM, Russia		$\bar{X}_{ref}$	$u^2(\bar{X}_{ref})$	$u_{\bar{X}_{ref}}$
	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$			
P <sub>1,0/50</sub> (W/kg)	0,3165	0,5	0,3173	0,218	0,3173	0,43	0,3138	0,325	0,3164	0,52	0,3164	0,0229	0,1514
P <sub>1,3/50</sub> (W/kg)	0,52	0,5	0,5232	0,229	0,522	0,44	0,517	0,325	0,5222	0,42	0,5213	0,0231	0,1518
P <sub>1,5/50</sub> (W/kg)	0,6985	0,5	0,7041	0,227	0,705	0,445	0,697	0,325	0,6996	0,42	0,7016	0,0229	0,1515
P <sub>1,7/50</sub> (W/kg)	1,0073	0,5	1,0154	0,414	1,018	0,51	1,008	0,38	1,001	0,36	1,0089	0,0353	0,1879
P <sub>1,8/50</sub> (W/kg)	1,3598	0,5	1,3719	0,634	1,374	0,895	1,371	0,465	1,3717	0,36	1,3693	0,0498	0,2232
P <sub>1,0/60</sub> (W/kg)			0,4108	0,214	0,403	0,43	0,4051	0,325	0,4041	0,42	0,4076	0,0236	0,1536
P <sub>1,3/60</sub> (W/kg)			0,6795	0,221	0,6697	0,43	0,671	0,325	0,6701	0,42	0,6749	0,0244	0,1561
P <sub>1,5/60</sub> (W/kg)			0,9143	0,23	0,9035	0,43	0,905	0,325	0,9055	0,38	0,9092	0,0246	0,1567
P <sub>1,7/60</sub> (W/kg)	1,3036	0,5	1,3054	0,414	1,2925	0,47	1,297	0,38	1,2983	0,36	1,2992	0,0345	0,1857
P <sub>1,8/60</sub> (W/kg)	1,7431	0,5	1,745	0,63	1,7453	0,845	1,747	0,465	1,7466	0,36	1,7457	0,0494	0,2222
30/50 (T)	1,5066	0,5	1,5027	0,133	1,4951	0,3			1,4999	0,52	1,5016	0,0133	0,1152
100/50 (T)	1,7288	0,5	1,7356	0,121	1,736	0,27	1,738	0,225	1,7336	0,36	1,7357	0,0088	0,0939
500/50 (T)	1,8449	0,5	1,8449	0,119	1,8456	0,265	1,846	0,225	1,8453	0,24	1,8452	0,0079	0,0891
1000/50 (T)	1,8855	0,5	1,8843	0,117	1,8875	0,265	1,885	0,225	1,8839	0,24	1,8847	0,0078	0,0882
1500/50 (T)	1,9095	0,5	1,9071	0,121	1,909	0,265	1,908	0,225	1,908	0,24	1,9077	0,0081	0,0899
30/60 (T)	1,4799	0,5	1,4909	0,134	1,4937	0,3			1,4929	0,52	1,4908	0,0134	0,1159
100/60 (T)	1,7296	0,5	1,7377	0,121	1,736	0,27	1,738	0,225	1,7359	0,36	1,7371	0,0088	0,0939
500/60 (T)	1,8452	0,5	1,8468	0,119	1,8477	0,265	1,846	0,225	1,8464	0,24	1,8467	0,0079	0,0891
1000/60 (T)	1,8851	0,5	1,8862	0,117	1,8834	0,265	1,885	0,225	1,8856	0,24	1,8856	0,0078	0,0882
1500/60 (T)	1,9085	0,5	1,909	0,12	1,9054	0,265	1,908	0,225	1,9081	0,24	1,9083	0,0080	0,0895

Table 4. The results of measurements and a standard uncertainty of measurement results of the ring sample □ 18

Parameter	CMI, Czech Republic		PTB, Germany		INRIM, Italy		NPL, United Kingdom		UNIIM, Russia		$\bar{X}_{ref}$	$u^2(\bar{X}_{ref})$	$u_{\bar{X}_{ref}}$
	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$			
P <sub>1,0/50</sub> (W/kg)	0,426	0,50	0,432	0,672	0,430	0,430	0,430	0,550	0,4332	0,76	0,4297	0,0600	0,2450
P <sub>1,3/50</sub> (W/kg)	0,716	0,50	0,725	0,675	0,723	0,451	0,722	0,550	0,7279	0,62	0,7222	0,0588	0,2424
P <sub>1,5/50</sub> (W/kg)	1,000	0,50	1,007	0,705	1,006	0,520	1,004	0,650	1,0042	0,58	1,0039	0,0664	0,2578
P <sub>1,7/50</sub> (W/kg)	1,471	0,50	1,461	0,821	1,469	1,185	1,459	1,300	1,4585	0,52	1,4642	0,0954	0,3088
P <sub>1,8/50</sub> (W/kg)	1,837	0,50	1,862	0,859	1,863	1,940	1,863	1,300	1,8607	0,64	1,8500	0,1156	0,3399
P <sub>1,0/60</sub> (W/kg)	0,565	0,50	0,569	0,668	0,568	0,430	0,568	0,550	0,5720	0,64	0,5680	0,0575	0,2398
P <sub>1,3/60</sub> (W/kg)	0,949	0,50	0,956	0,680	0,954	0,451	0,953	0,550	0,9593	0,64	0,9536	0,0594	0,2438
P <sub>1,5/60</sub> (W/kg)	1,317	0,50	1,324	0,695	1,323	0,485	1,320	0,650	1,3288	0,58	1,3220	0,0639	0,2527
P <sub>1,7/60</sub> (W/kg)	1,898	0,50	1,905	0,787	1,918	1,090	1,902	1,300	1,9053	0,52	1,9033	0,0931	0,3051
P <sub>1,0/400</sub> (W/kg)			11,447	0,672	11,405	0,430			11,4618	0,44	11,4352	0,0782	0,2796
P <sub>1,3/400</sub> (W/kg)			20,070	0,698	20,165	0,440			20,1480	0,46	20,1419	0,0837	0,2894
P <sub>1,5/400</sub> (W/kg)			28,960	0,725	28,953	0,451			28,7930	0,46	28,8887	0,0866	0,2943
P <sub>1,7/400</sub> (W/kg)			42,580	0,775	42,188	0,725			42,3240	1,44	42,3654	0,2469	0,4969
P <sub>0,5/1000</sub> (W/kg)	13,959	0,70	14,138	0,665	13,680	0,860			14,1460	0,92	14,0108	0,1463	0,3825
30/50 (T)	1,329	0,50	1,333	0,292	1,334	0,520			1,3289	0,24	1,3308	0,0272	0,1649
100/50 (T)	1,552	0,50	1,557	0,161	1,557	0,270	1,558	0,225	1,5550	0,24	1,5565	0,0107	0,1035
500/50 (T)	1,680	0,50	1,688	0,180	1,687	0,260	1,689	0,225	1,6876	0,24	1,6876	0,0115	0,1074
1000/50 (T)	1,755	0,50	1,758	0,165	1,759	0,260	1,758	0,225	1,7570	0,24	1,7579	0,0108	0,1039
1500/50 (T)	1,802	0,50	1,802	0,166	1,803	0,260	1,802	0,225	1,8014	0,24	1,8020	0,0108	0,1041
30/60 (T)	1,294	0,50	1,294	0,506	1,286	0,520			1,2938	0,24	1,2929	0,0345	0,1858
100/60 (T)	1,552	0,50	1,558	0,167	1,558	0,270	1,558	0,225	1,5547	0,24	1,5571	0,0110	0,1050
500/60 (T)	1,679	0,50	1,690	0,165	1,687	0,260	1,688	0,225	1,6889	0,24	1,6882	0,0108	0,1039
1000/60 (T)	1,753	0,50	1,759	0,165	1,761	0,260	1,758	0,225	1,7584	0,44	1,7590	0,0124	0,1115
1500/60 (T)	1,800	0,50	1,803	0,166	1,802	0,260	1,801	0,225	1,8031	0,44	1,8022	0,0125	0,1118
30/400 (T)	0,307	0,60	0,336	0,892	0,317	0,520			0,3149	0,32	0,3156	0,0571	0,2391
100/400 (T)	1,269	0,60	1,272	0,409	1,270	0,520			1,2716	0,34	1,2710	0,0474	0,2177
500/400 (T)	1,673	0,60	1,680	0,161	1,682	0,260			1,6803	0,30	1,6802	0,0149	0,1219
30/1000 (T)	0,153	0,60	0,159	0,879	0,151	0,520			0,1544	0,46	0,1533	0,0800	0,2829

Table 5. The results of measurements and a standard uncertainty of measurement results of the ring sample  $\square 1002$

Parameter	CMI, Czech Republic		PTB, Germany		INRIM, Italy		NPL, United Kingdom		UNIIM, Russia		$\bar{X}_{ref}$	$u^2(\bar{X}_{ref})$	$u_{\bar{X}_{ref}}$
	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$	X	$u_x, \%$			
P <sub>1,0/50</sub> (W/kg)			1,2001	0,3	1,2113	0,525	1,201	0,325	1,2107	0,34	1,2044	0,0304	0,1745
P <sub>1,1/50</sub> (W/kg)	1,4191	0,5	1,4242	0,302	1,44	0,57	1,425	0,325	1,4276	0,38	1,4259	0,0290	0,1704
P <sub>1,3/50</sub> (W/kg)	1,9594	0,5	1,9583	0,311	1,9775	0,6	1,96	0,325	1,962	0,42	1,9612	0,0310	0,1761
P <sub>1,5/50</sub> (W/kg)	2,752	0,5	2,7576	0,352	2,777	0,72	2,759	0,375	2,7551	0,22	2,7570	0,0239	0,1547
P <sub>1,6/50</sub> (W/kg)	3,394	0,5	3,391	0,383	3,432	1,485	3,391	0,375	3,3931	0,64	3,3927	0,0480	0,2191
P <sub>1,0/60</sub> (W/kg)			1,4973	0,3	1,5171	0,485	1,5	0,325	1,5035	0,36	1,5021	0,0307	0,1753
P <sub>1,1/60</sub> (W/kg)	1,7693	0,5	1,7773	0,298			1,78	0,325	1,7835	0,38	1,7785	0,0316	0,1777
P <sub>1,3/60</sub> (W/kg)			2,4432	0,311	2,4714	0,57	2,448	0,325	2,4517	0,44	2,4495	0,0357	0,1888
P <sub>1,5/60</sub> (W/kg)			3,434	0,349	3,474	0,67	3,436	0,375	3,4346	0,26	3,4375	0,0309	0,1758
P <sub>1,6/60</sub> (W/kg)			4,206	0,404	4,2588	1,4	4,216	0,375	4,2034	0,28	4,2084	0,0377	0,1942
100/50 (T)	0,9746	0,5	0,9714	0,185	0,967	0,395			0,9696	0,24	0,9706	0,0175	0,1325
200/50 (T)	1,2734	0,5	1,273	0,126	1,2728	0,295	1,278	0,225	1,2709	0,24	1,2735	0,0087	0,0930
500/50 (T)	1,4557	0,5	1,4565	0,103	1,4543	0,265	1,458	0,225	1,4539	0,24	1,4562	0,0067	0,0818
1000/50 (T)	1,5227	0,5	1,5258	0,105	1,523	0,26	1,526	0,225	1,5232	0,26	1,5252	0,0069	0,0833
100/60 (T)	0,9687	0,5	0,9704	0,186	0,964	0,395	0,979	0,26	0,9614	0,44	0,9710	0,0169	0,1299
200/60 (T)	1,2728	0,5	1,2733	0,126	1,2712	0,295	1,277	0,225	1,27	0,24	1,2732	0,0087	0,0930
500/60 (T)	1,4538	0,5	1,4575	0,103	1,4532	0,265	1,458	0,225	1,4537	0,24	1,4566	0,0067	0,0818
1000/60 (T)	1,5209	0,5	1,5271	0,105	1,5242	0,26	1,527	0,225	1,5216	0,24	1,5260	0,0068	0,0826

Table 6. The results of calculation of the equivalence of measurement standards for CRM 2002-80 ■ 1

Parameter	CMI, Czech Republic			PTB, Germany			INRIM, Italy			NPL, United Kingdom			UNIIM, Russia		
	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$
P <sub>1,0/50</sub> (W/kg)				0,0005	0,2529	0,0933	0,0114	0,5521	1,0298	-0,0056	0,3600	0,7817	0,0003	0,5426	0,0251
P <sub>1,15/50</sub> (W/kg)	-0,0099	0,2838	1,7428	0,0001	0,2434	0,0224	0,0105	0,5953	0,8826	-0,0045	0,3516	0,6386	0,0031	0,6148	0,2528
P <sub>1,3/50</sub> (W/kg)				0,0008	0,2965	0,1425	0,0102	0,6428	0,7969	-0,0038	0,3667	0,5120	-0,0010	0,4530	0,1054
P <sub>1,5/50</sub> (W/kg)				0,0044	0,2985	0,7335	0,0008	0,8381	0,0465	-0,0112	0,4132	1,3579	0,0006	0,3996	0,0725
P <sub>1,0/60</sub> (W/kg)				0,0005	0,2517	0,0952	0,0166	0,5037	1,6456	-0,0074	0,3591	1,0331	-0,0034	0,5228	0,3271
P <sub>1,1/60</sub> (W/kg)				0,0003	0,2561	0,0672	0,0131	0,5717	1,1495	-0,0049	0,3605	0,6734	-0,0015	0,5238	0,1390
P <sub>1,3/60</sub> (W/kg)				0,0006	0,2913	0,0945	0,0187	0,6026	1,5474	-0,0053	0,3638	0,7351	-0,0018	0,3954	0,2339
P <sub>1,5/60</sub> (W/kg)				0,0037	0,2946	0,6329	0,0164	0,8382	0,9800	-0,0146	0,4132	1,7631	0,0019	0,4178	0,2308
100/50 (T)				-0,0005	0,1801	0,1452	-0,0068	0,3109	1,0974	0,0062	0,2831	1,0910	0,0058	0,6104	0,4733
200/50 (T)				0,0000	0,1555	0,0033	-0,0032	0,3060	0,5211	0,0018	0,2453	0,3690	0,0003	0,4703	0,0330
500/50 (T)	-0,0051	0,2650	0,9579	0,0001	0,1463	0,0421	-0,0022	0,2839	0,3833	0,0012	0,2416	0,2532	-0,0005	0,3900	0,0611
1000/50 (T)	-0,0043	0,2647	0,8035	0,0002	0,1466	0,0840	-0,0024	0,2742	0,4293	0,0007	0,2412	0,1547	0,0002	0,3316	0,0371
2500/50 (T)	-0,0029	0,2644	0,5441	-0,0004	0,1453	0,1299	-0,0003	0,2739	0,0507	0,0014	0,2409	0,2952	0,0003	0,3121	0,0517
100/60 (T)				0,0002	0,1811	0,0685	-0,0101	0,3110	1,6158	0,0058	0,2833	1,0322	0,0074	0,6105	0,6101
200/60 (T)				0,0007	0,1544	0,2160	-0,0067	0,3059	1,1006	0,0017	0,2451	0,3401	0,0002	0,4702	0,0178
500/60 (T)	-0,0043	0,2649	0,8182	0,0004	0,1453	0,1259	-0,0018	0,2838	0,3232	0,0004	0,2414	0,0757	-0,0013	0,3899	0,1711
1000/60 (T)	-0,0025	0,2644	0,4778	0,0004	0,1445	0,1291	-0,0022	0,2739	0,4065	0,0007	0,2409	0,1397	-0,0008	0,3314	0,1248
2500/60 (T)	-0,0013	0,2644	0,2476	0,0002	0,1453	0,0655	0,0000	0,2739	0,0018	-0,0004	0,2409	0,0850	-0,0005	0,3121	0,0817

Table 7. The results of calculation of the equivalence of measurement standards for CRM 10271-2013 ■ 2

Parameter	CMI, Czech Republic			PTB, Germany			INRIM, Italy			NPL, United Kingdom			UNIIM, Russia		
	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$
P <sub>1.0/50</sub> (W/kg)	0,0001	0,5224	0,0105	0,0009	0,2654	0,1713	0,0009	0,4559	0,0997	-0,0026	0,3585	0,3613	0,0000	0,5416	0,0009
P <sub>1.3/50</sub> (W/kg)	-0,0013	0,5225	0,1223	0,0019	0,2748	0,3498	0,0007	0,4655	0,0776	-0,0043	0,3587	0,5963	0,0009	0,4466	0,1032
P <sub>1.5/50</sub> (W/kg)	-0,0031	0,5224	0,2932	0,0025	0,2729	0,4648	0,0034	0,4701	0,3656	-0,0046	0,3586	0,6363	-0,0020	0,4465	0,2199
P <sub>1.7/50</sub> (W/kg)	-0,0016	0,5341	0,1475	0,0065	0,4546	0,7175	0,0091	0,5435	0,8393	-0,0009	0,4239	0,1033	-0,0079	0,4061	0,9697
P <sub>1.8/50</sub> (W/kg)	-0,0095	0,5475	0,8708	0,0026	0,6721	0,1908	0,0047	0,9224	0,2528	0,0017	0,5158	0,1613	0,0024	0,4236	0,2791
P <sub>1.0/60</sub> (W/kg)				0,0032	0,2634	0,6007	-0,0046	0,4566	0,5076	-0,0025	0,3595	0,3526	-0,0035	0,4472	0,3952
P <sub>1.3/60</sub> (W/kg)				0,0046	0,2706	0,8413	-0,0052	0,4575	0,5735	-0,0039	0,3606	0,5473	-0,0048	0,4481	0,5409
P <sub>1.5/60</sub> (W/kg)				0,0051	0,2783	0,9153	-0,0057	0,4577	0,6232	-0,0042	0,3608	0,5827	-0,0037	0,4111	0,4506
P <sub>1.7/60</sub> (W/kg)	0,0044	0,5334	0,4084	0,0062	0,4537	0,6784	-0,0067	0,5054	0,6672	-0,0022	0,4229	0,2652	-0,0009	0,4051	0,1165
P <sub>1.8/60</sub> (W/kg)	-0,0026	0,5471	0,2387	-0,0007	0,6680	0,0533	-0,0004	0,8737	0,0235	0,0013	0,5153	0,1250	0,0009	0,4230	0,1050
30/50 (T)	0,0050	0,5131	0,4825	0,0011	0,1760	0,2987	-0,0065	0,3214	1,0189				-0,0017	0,5326	0,1642
100/50 (T)	-0,0069	0,5087	0,6772	-0,0001	0,1531	0,0295	0,0003	0,2859	0,0541	0,0023	0,2438	0,4737	-0,0021	0,3720	0,2809
500/50 (T)	-0,0003	0,5079	0,0302	-0,0003	0,1487	0,1032	0,0004	0,2796	0,0703	0,0008	0,2420	0,1639	0,0001	0,2560	0,0182
1000/50 (T)	0,0008	0,5077	0,0743	-0,0004	0,1465	0,1521	0,0028	0,2793	0,4930	0,0003	0,2417	0,0526	-0,0008	0,2557	0,1654
1500/50 (T)	0,0018	0,5080	0,1804	-0,0006	0,1508	0,1879	0,0013	0,2798	0,2382	0,0003	0,2423	0,0688	0,0003	0,2563	0,0650
30/60 (T)	-0,0109	0,5132	1,0644	0,0001	0,1771	0,0208	0,0029	0,3216	0,4468				0,0021	0,5328	0,1946
100/60 (T)	-0,0075	0,5087	0,7409	0,0006	0,1531	0,1832	-0,0011	0,2859	0,1992	0,0009	0,2438	0,1766	-0,0012	0,3720	0,1665
500/60 (T)	-0,0015	0,5079	0,1448	0,0001	0,1487	0,0436	0,0010	0,2796	0,1841	-0,0007	0,2420	0,1385	-0,0003	0,2560	0,0528
1000/60 (T)	-0,0005	0,5077	0,0482	0,0006	0,1465	0,2083	-0,0022	0,2793	0,3920	-0,0006	0,2417	0,1220	0,0000	0,2557	0,0021
1500/60 (T)	0,0002	0,5079	0,0207	0,0007	0,1497	0,2372	-0,0029	0,2797	0,5166	-0,0003	0,2422	0,0598	-0,0002	0,2562	0,0370



Table 8. The results of calculation of the equivalence of measurement standards for ring sample □ 18

Parameter	CMI, Czech Republic			PTB, Germany			INRIM, Italy			NPL, United Kingdom			UNIIM, Russia		
	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$
P <sub>1,0/50</sub> (W/kg)	-0,0035	0,5568	0,3130	0,0020	0,7153	0,1408	0,0003	0,4949	0,0317	0,0005	0,6021	0,0427	0,0035	0,7985	0,2200
P <sub>1,3/50</sub> (W/kg)	-0,0062	0,5557	0,5596	0,0032	0,7172	0,2218	0,0008	0,5120	0,0763	-0,0002	0,6010	0,0182	0,0057	0,6657	0,4267
P <sub>1,5/50</sub> (W/kg)	-0,0035	0,5625	0,3118	0,0026	0,7506	0,1726	0,0021	0,5804	0,1802	0,0001	0,6992	0,0066	0,0003	0,6347	0,0230
P <sub>1,7/50</sub> (W/kg)	0,0063	0,5877	0,5366	-0,0032	0,8772	0,1820	0,0051	1,2246	0,2085	-0,0052	1,3362	0,1943	-0,0057	0,6048	0,4707
P <sub>1,8/50</sub> (W/kg)	-0,0135	0,6046	1,1144	0,0120	0,9238	0,6508	0,0133	1,9696	0,3383	0,0133	1,3437	0,4958	0,0107	0,7247	0,7399
P <sub>1,0/60</sub> (W/kg)	-0,0032	0,5545	0,2854	0,0006	0,7097	0,0447	0,0002	0,4923	0,0239	0,0000	0,6000	0,0029	0,0040	0,6834	0,2952
P <sub>1,3/60</sub> (W/kg)	-0,0046	0,5563	0,4172	0,0024	0,7224	0,1633	0,0004	0,5127	0,0350	-0,0006	0,6016	0,0533	0,0057	0,6849	0,4132
P <sub>1,5/60</sub> (W/kg)	-0,0052	0,5602	0,4648	0,0016	0,7395	0,1077	0,0005	0,5469	0,0450	-0,0020	0,6974	0,1439	0,0068	0,6327	0,5368
P <sub>1,7/60</sub> (W/kg)	-0,0053	0,5857	0,4548	0,0017	0,8441	0,0991	0,0144	1,1319	0,6349	-0,0013	1,3353	0,0497	0,0020	0,6029	0,1636
P <sub>1,0/400</sub> (W/kg)				0,0118	0,7279	0,8095	-0,0302	0,5129	2,9454				0,0266	0,5213	2,5496
P <sub>1,3/400</sub> (W/kg)				-0,0719	0,7556	4,7610	0,0231	0,5266	2,1887				0,0061	0,5434	0,5569
P <sub>1,5/400</sub> (W/kg)				0,0713	0,7825	4,5589	0,0643	0,5385	5,9739				-0,0957	0,5461	8,7583
P <sub>1,7/400</sub> (W/kg)				0,2146	0,9206	11,6574	-0,1774	0,8790	10,0891				-0,0414	1,5233	1,3575
P <sub>0,5/1000</sub> (W/kg)	-0,0518	0,7977	3,2483	0,1272	0,7671	8,2890	-0,3308	0,9412	17,5741				0,1352	0,9963	6,7838
30/50 (T)	-0,0023	0,5265	0,2169	0,0026	0,3353	0,3901	0,0030	0,5455	0,2765				-0,0019	0,2912	0,3235
100/50 (T)	-0,0041	0,5106	0,4048	0,0002	0,1914	0,0435	0,0006	0,2891	0,0980	0,0015	0,2476	0,2961	-0,0015	0,2614	0,2934
500/50 (T)	-0,0072	0,5114	0,7034	0,0005	0,2096	0,1207	-0,0010	0,2813	0,1767	0,0014	0,2493	0,2820	0,0000	0,2629	0,0011
1000/50 (T)	-0,0026	0,5107	0,2526	0,0000	0,1950	0,0051	0,0015	0,2800	0,2715	0,0001	0,2478	0,0242	-0,0009	0,2615	0,1682
1500/50 (T)	0,0000	0,5107	0,0044	-0,0001	0,1960	0,0139	0,0008	0,2801	0,1509	-0,0001	0,2479	0,0110	-0,0006	0,2616	0,1060
30/60 (T)	0,0006	0,5334	0,0579	0,0015	0,5390	0,1408	-0,0066	0,5522	0,5960				0,0009	0,3035	0,1512
100/60 (T)	-0,0050	0,5109	0,4940	0,0010	0,1973	0,2414	0,0009	0,2897	0,1471	0,0009	0,2483	0,1717	-0,0024	0,2620	0,4672
500/60 (T)	-0,0095	0,5107	0,9342	0,0014	0,1950	0,3483	-0,0012	0,2800	0,2218	-0,0002	0,2478	0,0488	0,0007	0,2615	0,1258
1000/60 (T)	-0,0065	0,5123	0,6298	0,0003	0,1991	0,0872	0,0023	0,2829	0,4149	-0,0010	0,2511	0,1897	-0,0006	0,4539	0,0609
1500/60 (T)	-0,0019	0,5123	0,1823	0,0011	0,2001	0,2827	-0,0004	0,2830	0,0651	-0,0017	0,2512	0,3320	0,0009	0,4540	0,1026
30/400 (T)	-0,0083	0,6459	0,6434	0,0207	0,9235	1,1202	0,0011	0,5723	0,0951	-0,3156	0,2391	66,0118	-0,0007	0,3994	0,0890
100/400 (T)	-0,0023	0,6383	0,1781	0,0006	0,4633	0,0677	-0,0008	0,5637	0,0686	-1,2710	0,2177	291,9401	0,0006	0,4037	0,0777
500/400 (T)	-0,0075	0,6123	0,6097	-0,0002	0,2020	0,0411	0,0017	0,2872	0,3019	-1,6802	0,1219	688,9733	0,0001	0,3238	0,0207
30/1000 (T)	0,0004	0,6633	0,0302	0,0059	0,9234	0,3172	-0,0028	0,5920	0,2401	-0,1533	0,3223	23,7904	0,0011	0,5400	0,0979

Table 9. The results of calculation of the equivalence of measurement standards for ring sample  $\square 1002$

Parameter	CMI, Czech Republic			PTB, Germany			INRIM, Italy			NPL, United Kingdom			UNIIM, Russia		
	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$	$d_i$	$u(d_i)$	$E_n$
$P_{1,0/50}$ (W/kg)				-0,0043	0,3470	0,6176	0,0069	0,5532	0,6248	-0,0034	0,3689	0,4591	0,0063	0,3821	0,8260
$P_{1,1/50}$ (W/kg)	-0,0068	0,5282	0,6459	-0,0017	0,3468	0,2485	0,0141	0,5949	1,1830	-0,0009	0,3670	0,1258	0,0017	0,4165	0,2013
$P_{1,3/50}$ (W/kg)	-0,0018	0,5301	0,1735	-0,0029	0,3574	0,4112	0,0163	0,6253	1,3002	-0,0012	0,3696	0,1676	0,0008	0,4554	0,0835
$P_{1,5/50}$ (W/kg)	-0,0050	0,5234	0,4740	0,0006	0,3845	0,0830	0,0200	0,7364	1,3605	0,0020	0,4057	0,2513	-0,0019	0,2690	0,3460
$P_{1,6/50}$ (W/kg)	0,0013	0,5459	0,1177	-0,0017	0,4413	0,1944	0,0393	1,5011	1,3085	-0,0017	0,4343	0,1975	0,0004	0,6765	0,0284
$P_{1,0/60}$ (W/kg)				-0,0048	0,3475	0,6967	0,0150	0,5157	1,4503	-0,0021	0,3693	0,2900	0,0014	0,4004	0,1696
$P_{1,1/60}$ (W/kg)	-0,0092	0,5307	0,8624	-0,0012	0,3470	0,1662				0,0015	0,3704	0,2088	0,0050	0,4195	0,6015
$P_{1,3/60}$ (W/kg)				-0,0063	0,3638	0,8630	0,0219	0,6005	1,8253	-0,0015	0,3759	0,1968	0,0022	0,4788	0,2319
$P_{1,5/60}$ (W/kg)				-0,0035	0,3908	0,4439	0,0365	0,6927	2,6369	-0,0015	0,4142	0,1774	-0,0029	0,3139	0,4571
$P_{1,6/60}$ (W/kg)				-0,0024	0,4483	0,2731	0,0504	1,4134	1,7812	0,0076	0,4223	0,8941	-0,0050	0,3408	0,7407
100/50 (T)	0,0040	0,5172	0,3885	0,0008	0,2275	0,1799	-0,0036	0,4166	0,4298				-0,0010	0,2741	0,1790
200/50 (T)	-0,0001	0,5086	0,0131	-0,0005	0,1566	0,1702	-0,0007	0,3093	0,1185	0,0045	0,2435	0,9174	-0,0026	0,2574	0,5115
500/50 (T)	-0,0005	0,5066	0,0459	0,0003	0,1315	0,1272	-0,0019	0,2773	0,3363	0,0018	0,2394	0,3831	-0,0023	0,2535	0,4468
1000/50 (T)	-0,0025	0,5069	0,2453	0,0006	0,1340	0,2287	-0,0022	0,2730	0,4005	0,0008	0,2399	0,1695	-0,0020	0,2730	0,3638
100/60 (T)	-0,0023	0,5166	0,2183	-0,0006	0,2269	0,1224	-0,0070	0,4158	0,8364	0,0080	0,2906	1,3840	-0,0096	0,4588	1,0414
200/60 (T)	-0,0004	0,5086	0,0404	0,0001	0,1566	0,0285	-0,0020	0,3093	0,3250	0,0038	0,2435	0,7782	-0,0032	0,2574	0,6237
500/60 (T)	-0,0028	0,5066	0,2780	0,0009	0,1315	0,3358	-0,0034	0,2773	0,6160	0,0014	0,2394	0,2889	-0,0029	0,2535	0,5752
1000/60 (T)	-0,0051	0,5068	0,5006	0,0011	0,1336	0,4216	-0,0018	0,2728	0,3250	0,0010	0,2397	0,2141	-0,0044	0,2538	0,8616

Ural Scientific Research  
Institute of Metrology  
(FGUP «UNIIM»), Russia

Malygin **И.И.**

---

signature

Physikalisch-Technische  
Bundesanstalt (PTB), Germany

Martin Albrecht

---

signature

Czech Metrology Institute  
(CMI), Czech Republic

Josef Kupec

---

signature

National Physical Laboratory  
(NPL), United Kingdom

Steven Turner

---

signature

Istituto Nazionale di Ricerca Metrologica  
(INRIM), Italy

Carlo Appino

---

signature